

AUG 18 1997

K 971874

**510(k) Summary of Safety and Effectiveness  
Sharplan Lasers, Inc. Model 5000 Alexandrite Laser System**

In response to the Safe Medical Devices Act of 1990, the following is a summary of the safety and effectiveness information upon which the substantial equivalence determination is based.

The safety and effectiveness of Sharplan Model 5000 Alexandrite Laser System is based upon a determination of the substantial equivalence as well as the safety and effectiveness of its predicate device which is the Cynosure PhotoGenica LP Dermatological Vascular Lesion Laser.

1. Sharplan Lasers, Inc.  
1 Pearl Court  
Allendale, NJ 07401  
George J. Hattub, Director of Regulatory Affairs/Quality Assurance  
May 16, 1997
2. **Model:** Sharplan Model 5000 Alexandrite Laser System
3. **Predicate Device:** The Cynosure PhotoGenica LP Dermatological Vascular Lesion Laser (K963094)
4. **Description:** The Sharplan Model Alexandrite Laser System is a medical device which capable of emitting an invisible pulsed treatment laser beam at a wavelength of 755 nm under the guidance of an visible aiming beam. This laser can be utilized in either the continuous or timed exposure modes of operation
5. The Sharplan Model 5000 Alexandrite Laser System is intended for use in dermatology for the treatment of vascular lesions. No new indications were sought in this premarket notification and no clinical data was presented.

**510(k) Summary of Safety and Effectiveness**  
**Sharplan Lasers, Inc. Model 5000 Alexandrite Laser System**  
**(continued)**

6. From both a design and clinical perspective, the predicate and candidate laser devices, are of the same technology and have the same intended use. Based upon an analysis of the overall performance characteristics for the devices, Sharplan Lasers, Inc. believes that no significant differences exist. Therefore, the Sharplan Model 5000 Alexandrite Surgical Laser should not raise any concerns regarding its overall safety or effectiveness.

**Advisory:** This information was prepared for the sole purpose of compliance with the Safe Medical Devices Act of 1990. It does not imply that the procedures described herein can be performed with the equipment described without substantial risk of personal injury or death to patients due to operator error or in procedures requiring a high degree of skill.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration  
9200 Corporate Boulevard  
Rockville MD 20850

Mr. George J. Hattub  
Director, Regulatory Affairs/Quality Assurance  
Sharplan Lasers, Inc.  
33 Plan Way  
Warwick, Rhode Island 02886

AUG 18 1997

Re: K971874  
Trade Name: Sharplan Model 5000 Alexandrite Laser System  
Regulatory Class: II  
Product Code: GEX  
Dated: May 19, 1997  
Received: May 20, 1997

Dear Mr. Hattub:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

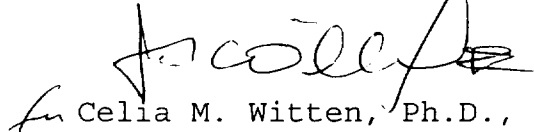
If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the current Good Manufacturing Practice requirement, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic (QS) inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

Page 2 - Mr. George J. Hattub

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4595. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its internet address "<http://www.fda.gov/cdrh/dsmamain.html>".

Sincerely yours,

A handwritten signature in black ink, appearing to read 'C. Witten', with a stylized flourish at the end.

Celia M. Witten, Ph.D., M.D.  
Director  
Division of General and  
Restorative Devices  
Office of Device Evaluation  
Center for Devices and  
Radiological Health

Enclosure

510(k) Number (If known): K 971874

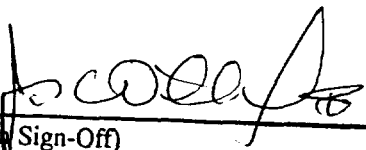
Device Name: Sharplan Model 5000 Alexandrite Laser System

Indications For Use:

The Sharplan Model 5000 Alexandrite Surgical Laser System is intended for use in dermatology for the treatment of vascular lesions.

(Please Do Not Write Below This Line - Continue on Another Page If Needed)

Concurrence of CDRH, Office of Device Evaluation (ODE)

  
(Division Sign-Off)  
Division of General Restorative Devices  
510(k) Number K971874

Prescription Use ☒  
(Per 21 CFR 801.109)

OR

Over-The-Counter Use ☐

(Optional Format 1-2-96)